

SEXUAL HEALTH COLLECTION KIT

A vaginal and extra-genital (throat and rectal) swab sample collection kit used for the collection and transportation of samples for laboratory analysis of sexually transmitted infections by nucleic acid technique (NAT)

This kit contains the materials required for either sample self-collection or collection by a health/social care professional.



For in vitro diagnostic use, sample self-collection









Important: Do not use kit if security seal is broken Keep out of reach of children



Do not re-use

Carefully read the

leaflet before use

enclosed instruction




For use by persons aged 18 and over

Sample collection instructions (Steps 1-29)

- Please ensure the kit is within expiry date and read these instructions carefully and completely before attempting to collect the sample.
- If your kit requires online activation, please follow the instructions provided by your healthcare organisation. If you need assistance please contact the healthcare organisation who arranged the test.

Your sample collection kit contents

Please check that the kit contains all of the items outlined below. Do not proceed with sample taking if any items are missing or damaged, contact the healthcare organisation who arranged your test for assistance.








Return security label

Sample label



Sample collection tube case






Return postal envelope





Collection kit outer box

THROAT SWAB SAMPLE COLLECTION






Clearly complete a sample collection tube label using a ball point pen with:


- Your First name
- Your Surname
- · Your Date of birth
- · Sample type: Throat



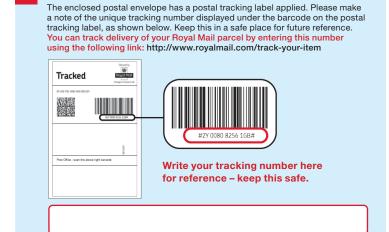



IMPORTANT SAMPLE TRACKING INFORMATION!





The sample collection tube case has been designed to provide a stable way of holding the swab collection tube whilst a sample is taken. Please insert the tube as shown, remove the cap and put it to one side whilst you take your sample. Take care not to spill any of the liquid the tube contains. **Do not touch** or pierce the foil top of the lid.







Carefully insert the swab into the mouth ensuring contact with the 5 key areas:

- Tonsil
- 2 Posterior wall
- 3 Uvula
- 4 Posterior wall
- 5 Tonsil

Please do not let the end of the swab touch other areas of the mouth.





Discard the stick end of the swab in a bin leaving the cotton end in the liquid. Screw the cap back onto the tube tightly.

> Place the tube into the protective packing case and firmly close




VAGINAL SWAB SAMPLE COLLECTION




Your First name

- Your Surname
- Your Date of birth
- · Sample type: Vaginal













Gently insert the swab about 5 cm into your vagina. Your fingers on the black line will stop you going in too far. If the swab does not slide easily, gently rotate it as you put it in. If it is too difficult, do not attempt to continue




Rotate the swab for 5 seconds (count to 5 slowly), making sure it touches the walls of your vagina. Carefully pull out the swab.



Discard the stick end of the swab in a bin leaving the cotton end in the liquid. Screw the cap back onto the tube tightly. Place the tube into the protective packing case and firmly close





RECTAL SWAB SAMPLE COLLECTION





- Your Surname • Your Date of birth Sample type: Rectal















IMPORTANT CHECKLIST

Before you return your sample please do the following:

- Place your completed request form supplied by your doctor/clinic into the postal envelope
- Make sure each swab specimen transport tube is labelled and is placed inside the protective packing case
- Place the protective case into the collection kit outer box
- Close the collection kit outer box firmly and apply the return security label to seal it
- Place the collection kit outer box into the return postal envelope
 - Check that you have taken note of your postal tracking number

You are now ready to seal the postal envelope. Please store at room temperature until posted.

Please post your sample to The Doctors Laboratory as soon as possible (ideally on same day or within 24 hours of sample collection) from ANY Royal Mail post box in the UK. No stamp is required within the UK.

If you need assistance please contact The Doctors Laboratory on 020 7307 7373 or email samples@tdlpathology.com.



We would welcome feedback on your experience of using this self-collection kit to help us improve our services. To complete a short online survey please scan the code or visit:

https://forms.office.com/r/SWWruqwKda

Warnings and precautions

- This kit is designed for use by persons aged 18 and over and upon request of a healthcare professional or healthcare organisation.
- Please consult with a healthcare professional for guidance on sample collection processes for adolescent and younger children.
- The kit should not be used by individuals lacking the physical or mental capacity to correctly follow the self-collection instructions. If you have problems or feel unwell or lightheaded during the collection process, please pause and if necessary, consult with your advising healthcare professional.
- If you have experienced recent pelvic pain, pain during or as a result of sexual intercourse and/or unusual vaginal discharge or odor please discuss this with your healthcare professional before collecting your sample.
- The Hologic transport buffer contains no substances which at their given concentration, are considered to be hazardous to health. In the case of contact with eyes, skin or mouth please and rinse thoroughly with clean water, if ingested please drink plenty of water and if any symptoms occur please consult a medical professional. In the case of spillages please wipe with absorbent paper and dispose in normal household waste. For further information please refer to safety datasheets which can be found at www.hologic.com or contact MolecularSupport@hologic.com.
- Samples arriving at the laboratory which show evidence of the below may
 - · Leaking sample/no liquid present in collection tube
 - . No swab inside the collection tube
 - . Two or more swabs inside the collection tube
 - Swab placed upside down in the collection tube
 - · Different swab type/brand to the one supplied
 - General damage
- The sample collection swab has a score line, which after sampling helps the swab break at the correct position when pressure is applied to allow it to fit in the collection tube. If this score line is broken, appears damaged or the swab arrives in two broken parts, do not use and request another kit from your healthcare organisation.
- Use with caution if allergic to nylon fibre and ABS (Acrylonitrile butadiene styrene) material. If any problems arise during the sample collection process please contact your healthcare organisation.
- The accuracy of your results may be compromised if you do not read and follow the instructions in full.
- Samples arriving at the laboratory which show signs of degradation or general damage or arrive after 60 days (Aptima swab) of sample taking may not be tested.
- Please note that some medicines or medicinal products may be considered interfering substances for certain biochemical or immunoassay investigations. Please consider the potential impact of interfering substances when interpreting results.
- Where appropriate, out of range, abnormal or positive test results deemed clinically significant should be confirmed with a confirmatory venous sample.

Materials required but not provided

- Test request form. This will be provided by your healthcare professional or healthcare organisation. Please complete the request form with your details as instructed.
- · Clean tissue paper

Laboratory Tests

- The tests and procedures undertaken by The Doctors Laboratory Limited are verified and performed in line with supplier product instructions for use and supported by additional validation data for use with self-collection procedures.
- Test results are provided in line with clinically approved results pathways, agreed between The Doctors Laboratory Limited and the patients designated healthcare professional or healthcare organisation.

KEY TO SYMBOLS

IVD

For in vitro diagnostic use





Catalogue number





Sterilized using



Biological risk. Biological sample, treat as potentially infectious

package is damaged



Distributor

Do not use if



Use by end of year-month



FU Authorised

Representative

Temperature limits: 4°-25°C

Caution, consult

accompanying

documents

Keep away

from sunlight

UK Conformity



EU Conformity



Assessed Do not re-use



Not made with natural rubber latex



Consult instructions for use



For use by persons aged 18 and over



Keep dry



REAL Digital International Limited, 2 Queensway, Croydon, Surrey, CRO 4BD, UK Website: www.real-digital.co.uk



Casus Europe BV, Lange Viestraat 2 B, 3511BK Utrecht, The Netherlands.



The Doctors Laboratory Limited

Distribution is restricted to regions in which the product is registered by the manufacturer.

© The Doctors Laboratory Limited, 2024, Illustrations: © Jag Mathary/Thin Air Productions RDI-IFU-054, TAP5109C/05-02-24/V12. Issue No. 2; Date 05/02/24.

Revision/Date		Change summary	
1	02/2023	Initial RDi product for UK market	
2	02/2024	RDi IVD product CE registration	

If any serious incident occurs in relation to the use of this kit, it should be reported to the manufacturer and the competent authority of the Member State in which the user and/or the patient is established.